ORIGINAL PAPER

Comparison of Osseointegration in Novel Laser-Textured and SLA Implants

Ralph Zarazir[1,2], Stephanie Mrad[3], Georges Aoun[4], Alain Abi Sleiman[1], Marianne Mousallem[5], Joseph Bassil[3]

[1]Attending Oral Surgeon, Military Medicine, Beirut, Lebanon

[2]Department of Restorative and Esthetic Dentistry, Faculty of Dental Medicine, Saint Joseph University of Beirut, Lebanon

[3]Department of Oral Surgery, Faculty of Dental Medicine, Saint Joseph University of Beirut, Lebanon

[4]Department of Oral Medicine and Maxillofacial Radiology, Faculty of Dental Medicine, Lebanese University, Beirut, Lebanon

[5]High Institute of Public Health, Saint Joseph University of Beirut, Lebanon

Corresponding author: Professor Georges Aoun, Department of Oral Medicine and Maxillofacial Radiology, Faculty of Dental Medicine, Lebanese University, Beirut, Lebanon. E-mail: dr.georgesaoun@gmail.com, ORCID ID: http://orcid.org/0000- 0001-5073-6882.

doi: 10.5455/aim.2023.31.137-140

ACTA INFORM MED. 2023 JUN 31(2): 137-140

Received: MAY 15, 2023

Accepted: JUN 25, 2023

ABSTRACT

Background: Osseointegration is defined as the direct structural and functional connection between neo-formed bone and dental implants. Among the parameters suggested to predominantly influencing the establishment of a successful osseointegration is the quality of the implant surface, which may enhance the strength and speed of this biomechanical process. **Objective:** The purpose of this study was to evaluate the ability of a novel laser-treated surface, compared to sandblasted, large-grit, acid-etched (SLA) surfaces, to enhance and accelerate implant integration in delayed implant placement. **Methods:** Thirty patients with two missing posterior teeth were enrolled in this study. Each patient received, at a randomly allocated site, an implant with a conventional SLA surface, and at a second site, an implant with laser-textured surface. A total of 60 tissue-level implants were subsequently placed. Implant stability (ISQ) was measured using resonance frequency analysis (RFA). ISQ was assessed at baseline (T0), 8 weeks (T1), and 12 weeks (T2) following implant placement. **Results:** There was a statistical difference in implant stability between laser-textured and SLA group at 12 weeks postoperatively. Implant stabilization showed a successful osseointegration with both surface types. **Conclusion:** Both laser and SLA surface treatments had positive impacts on implant stabilization following delayed placement. Laser-treated surfaces presented higher values of osseointegration at 3 months postoperatively.

Keywords: implant stability, implant surface, resonance frequency analysis, dental implant, laser-textured implants.

1. BACKGROUND

Osseointegration is defined as the direct structural and functional connection between neo-formed bone and dental implants without interposition of fibrous tissue (1). Several parameters have been suggested to predominantly influence the establishment of a successful osseointegration (2). Among these factors is the quality of the implant surface, which may enhance the strength and speed of this biomechanical process (3). Wennerberg et al. proposed a classification for surface roughness going from smooth (≤ 0,4 μm), to minimally rough or machined (0,5–1,0 μm), intermediately or moderately rough (1,0–2,0 μm), and rough (> 2,0 μm) (4). Implant roughness can be created by different treatment modalities such as sandblasting, acid etching, titanium plasma spraying, and hydroxyapatite coating (5). Sandblasted, large-grit, acid-etched (SLA) implants have demonstrated one of the most increased rates and degrees of osseointegration during the early phases of healing (6, 7).

Recently, a novel technology of surface treatment via robotic tools for laser ablation is being introduced. Laser-treated surfaces (LZ) have been suggested to enhance the biological properties of implants. This method consists of creating a mesh of well-defined, identical (in size and shape), symmetrically distributed, hemispherical micrometric pores. The resulting topography may increase cell attachment and bone differentiation, thus promoting more stable osseointegration (1). Implants treated with laser have also been proposed to significantly reduce bacterial adhesion and peri-implantitis risk (8, 9).

2. OBJECTIVE

The aim of this study is to compare the implant stability of LZ to SLA surfaces during osseointegration.

3. MATERIAL AND METHODS

Patient selection

This randomized controlled clinical trial was conducted between March 2021 and July 2022. Patients requiring the placement of two adjacent / contralateral implants in the same mandible (either superior or inferior) were selected. All participants signed an informed consent prior to any intervention.

The study population included thirty patients with two missing posterior teeth in the mandible or maxilla requiring implant-supported restorations. Patients who fulfilled the following inclusion criteria were enrolled in this study:

- Adult patients (above 21 years of age)
- Light or non-smokers (<10 cigarettes per day)
- Absence of systemic diseases (ASA 1 patients)
- Absence of osseous diseases that may affect peri-implant healing
- Absence of periodontal diseases and oral hygiene problems
- Sufficient bone width and length without previous ridge preservation nor bone augmentation procedures
- Adjacent or symmetrical contra-lateral implant sites.

Surgical procedure

All patients were asked to rinse with chlorhexidine 0.12% for one minute prior to surgery. Under local anesthesia infiltration (Articaine with adrenaline 1/100 000), a linear mid-crestal incision was made and a full-thickness flap was raised. Sites were prepared following the manufacturer's drilling sequence.

Implants from BIOMED® (Manufacturer: Dr. Ihde Dental AG, St. Gallen, SWITZERLAND) with grade 5 titanium alloy were used in the current study. Sites were randomly allocated to receive either a traditional implant from BIOMED®; double-sandblasted/acid-etched (SLA) or a laser-textured LZ implant (No-Itis® surface) from the same manufacturer. Each patient received two implants, both placed by the same surgeon. A total of sixty Tissue Level standard size, diameter, and length (4.1 x 9 mm) implants were placed. Implants were covered with transgingival healing caps and flaps were sutured.

Implant stability quotient (ISQ) was then measured by a single masked examiner with a resonance frequency analysis (RFA) device (Osstell ISQ; Integration Diagnostics AB, Gothenburg, SWEDEN). ISQ values were determined in duplicate and a third reading was taken in case of a difference greater than 2 ISQ between readings. Independent measurements were assessed at the buccal, palatal/lingual, occlusal, and proximal sides of each implant.

Postoperatively, patients were prescribed antibiotics (Amoxicillin 2g/day/7 days or, in case of allergies, Clindamycin 600mg/day/7 days), anti-inflammatories (Brufen 400mg/8h/3 days), and chlorhexidine mouth rinses (CHX 0.12%/twice a day/10days).

ISQ measurements were performed immediately after surgery (T0), at 8 weeks (T1) and 12 weeks (T2) postoperatively.

Statistical analysis

A descriptive analysis was first carried out. Quantitative variables are described by their minimum, maximum, mean, and standard deviation (SD). The paired-samples t-test was used to assess whether the mean ISQ values at Day 1 and week 12 of the SLA and LZ implants are significantly different. A P value of less than 0.05 was considered statistically significant. IBM SPSS Statistics 25 software was used for data analysis.

4. RESULTS

Twenty-seven participants (n = 27) were included in the study (3 patients were taken out of the study because of reasons related to implant failure or postoperative infection). ISQ values decrease between the day of insertion and the eighth week for both types of implants, then increase at the twelfth week. The ISQ values for SLA and LZ implants are presented in Table 1 and Figure 1.

Type of implant	Variable	Minimum	Maximum	Mean	SD
SLA	Mean D1	50.0	82.8	68.70	6.76
	Mean W8	56.4	73.0	67.71	4.26
	Mean W12	61.6	82.8	71.28	4.96
LZ	Mean D1	54.8	80.0	69.59	5.79
	Mean W8	56.6	76.2	67.37	4.79
	Mean W12	58.8	82.4	73.53	6.21

Table 1. ISQ values for LZ and SLA implants (n=27)

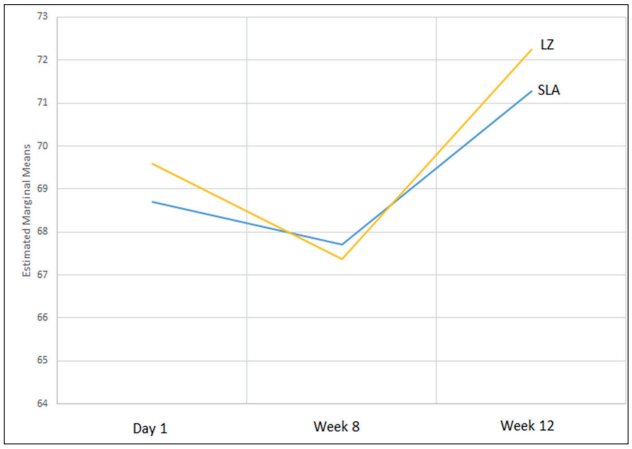

Figure 1. Mean ISQ at day 1, week 8, and week 12 for LZ and SLA implants (n=27)

Bivariate analyses showed that:

There was no statistically significant difference between the mean ISQ values of SLA and LZ implants on the day of placement (p-value = 0.479).

There was a statistically significant difference between the mean ISQ values of SLA and LZ implants at week 12 (p-value=0.003), with LZ implants having a significantly higher ISQ at week 12 (with a mean of 73.53 and a standard deviation of 6.21) than SLA implants (with a mean of 71.28 and a standard deviation of 4.96).

5. DISCUSSION

This randomized clinical study aimed to evaluate the potential of laser-treated surfaces to enhance implant healing and osseointegration when compared to standard SLA surfaces.

Several studies underlined the critical role of titanium implants' macro- and microtopography during the initial osseointegration phase (10, 11). Healing of dental implants is

a complex course that begins after insertion and continues during implant integration into the bone (11, 12). Surface treatment and roughness are considered as a main factor influencing the quality of dental implant integration (1, 13, 14). Several surface treatments have been evaluated in terms of neo formation and integration of bone around dental implants in early healing phases (15, 17).

Among these treatment modalities, micro-rough SLA implants are commonly presented to reduce osseointegration duration (1(). SLA surface is formed by a 0.25-0.5 mm corundum of coarse grit blasting followed by acid etching with hydrochloric and sulphuric acid (19). Preclinical studies showed higher bone-to-implant (BIC) and torque removal values with SLA implants compared to minimally rough surfaces (15, 20). Histological findings indicated that SLA surface can promote initial contact osteogenesis (at the implant surface) but also distance osteogenesis (at the exposed bone wall) (7). A comparative study between implant surfaces showed an increase in stability values after 4 weeks for SLA implants (21). In the current study, SLA implants exhibited a mean ISQ value of 68.70 at day one that kept slightly decreasing until the 8th week with an ISQ of 67.71, then started increasing to reach 71.28 at 12 weeks.

Innovative LZ implants display high biocompatibility with osteoblast cultures. Thus, this surface treatment may influence the osteogenic process, increase cell proliferation and differentiation, contribute to bone matrix synthesis, and enhance bone deposition at early osseointegration phases (22). On the other hand, LZ implants are characterized by a smooth surface, which was found to reduce the adsorption of bacterial adhesion proteins and the risk of peri-implantitis (8). In the current study, the stability of LZ implants over time was similar to that of SLA implants. LZ group showed a mean stability value of 69.59 at surgery day, 67.37 at 8 weeks, and 73.53 at 12 weeks.

There was no statistical difference in primary stability between both SLA and LZ implants. Thus, the implant micro-geometry and surface treatment did not have any influence on the primary stability. Implant stability continued to decrease up to the 8th week in both groups with a lower mean ISQ value in the LZ group. LZ were not able to promote faster osseointegration. However, the difference at 8 weeks was not statistically significant and the two groups were able to maintain relatively high ISQ values for loading at 8 weeks. Afterwards, ISQ values progressively increased in the SLA and LZ groups. At 12 weeks postoperatively, ISQ of the LZ implants showed significantly higher values than the SLA implants with a mean of 73.53 compared to a mean of 71.28. The difference between the two groups is a preliminary proof that this innovative laser treatment of implant surfaces may enhance osseointegration and achieve higher values of secondary stability. Further studies with larger samples are required to validate these results on the long-term.

6. CONCLUSION

LZ and SLA implants surfaces can both achieve successful osseointegration. Nevertheless, a higher secondary stability may be obtained with LZ implants.

REFERENCES

1. Smeets R, Stadlinger B, Schwarz F, Beck-Broichsitter B, Jung O, Precht C, et al. Impact of Dental Implant Surface Modifications on Osseointegration. Biomed Res Int. 2016;2016:6285620. doi: 10.1155/2016/6285620.
2. Sykaras N, Iacopino AM, Marker VA, Triplett RG, Woody RD. Implant materials, designs, and surface topographies: their effect on osseointegration. A literature review. Int J Oral Maxillofac Implants. 2000;15(5):675-90.
3. Albrektsson T, Brånemark PI, Hansson HA, Lindström J. Osseointegrated titanium implants. Requirements for ensuring a long-lasting, direct bone-to-implant anchorage in man. Acta Orthop Scand. 1981;52(2):155-70. doi: 10.3109/17453678108991776.
4. Wennerberg A, Albrektsson T. On implant surfaces: a review of current knowledge and opinions. Int J Oral Maxillofac Implants. 2010;25(1):63-74.
5. Novaes AB Jr, de Souza SL, de Barros RR, Pereira KK, Iezzi G, Piattelli A. Influence of implant surfaces on osseointegration. Braz Dent J. 2010;21(6):471-81. doi: 10.1590/s0103-64402010000600001.
6. Botticelli D, Berglundh T, Buser D, Lindhe J. Appositional bone formation in marginal defects at implants. Clin Oral Implants Res. 2003;14(1):1-9. doi: 10.1034/j.1600-0501.2003.140101.x.
7. Abrahamsson I, Berglundh T, Linder E, Lang NP, Lindhe J. Early bone formation adjacent to rough and turned endosseous implant surfaces. An experimental study in the dog. Clin Oral Implants Res. 2004;15(4):381-92. doi: 10.1111/j.1600-0501.2004.01082.x.
8. Motzfeld R, Covarrubias C, Gómez L, Bastias F, Maureira M. A comparative study on the microstructural and antibacterial properties of Laser-textured and SLA dental implants. Int J Interdiscip Dent 2021; 14(3):222-5. doi: 10.4067/S2452-55882021000300222.
9. Kokubo T, Kushitani H, Sakka S, Kitsugi T, Yamamuro T. Solutions able to reproduce in vivo surface-structure changes in bioactive glass-ceramic A-W. J Biomed Mater Res. 1990;24(6):721-34. doi: 10.1002/jbm.820240607.
10. Martin JY, Schwartz Z, Hummert TW, Schraub DM, Simpson J, Lankford J Jr, et al. Effect of titanium surface roughness on proliferation, differentiation, and protein synthesis of human osteoblast-like cells (MG63). J Biomed Mater Res. 1995;29(3):389-401. doi: 10.1002/jbm.820290314.
11. Cooper LF. A role for surface topography in creating and maintaining bone at titanium endosseous implants. J Prosthet Dent. 2000;84(5):522-34. doi: 10.1067/mpr.2000.111966.
12. Mustafa K, Wennerberg A, Wroblewski J, Hultenby K, Lopez BS, Arvidson K. Determining optimal surface roughness of TiO(2) blasted titanium implant material for attachment, proliferation and differentiation of cells derived from human mandibular alveolar bone. Clin Oral Implants Res. 2001;12(5):515-25. doi: 10.1034/j.1600-0501.2001.120513.x..
13. Tetè S, Mastrangelo F, Quaresima R, Vinci R, Sammartino G, Stuppia L, Gherlone E. Influence of novel nano-titanium implant surface on human osteoblast behavior and growth. Implant Dent. 2010;19(6):520-31. doi: 10.1097/ID.0b013e3182002eac.
14. Antonucci I, Iezzi I, Morizio E, Mastrangelo F, Pantalone A, Mattioli-Belmonte M, Gigante A, Salini V, Calabrese G, Tetè S, Palka G, Stuppia L. Isolation of osteogenic progenitors from human amniotic fluid using a single step culture protocol. BMC Biotechnol. 2009;16;9:9. doi: 10.1186/1472-6750-9-9.
15. Cochran DL, Schenk RK, Lussi A, Higginbottom FL, Buser D. Bone response to unloaded and loaded titanium implants with

a sandblasted and acid-etched surface: a histometric study in the canine mandible. J Biomed Mater Res. 1998;40(1):1-11. doi: 10.1002/(sici)1097-4636(199804)40:1<1::aid-jbm1>3.0.co;2-q.

16. Park BS, Heo SJ, Kim CS, Oh JE, Kim JM, Lee G, et al. Effects of adhesion molecules on the behavior of osteoblast-like cells and normal human fibroblasts on different titanium surfaces. J Biomed Mater Res A. 2005;74(4):640-51. doi: 10.1002/jbm.a.30326.
17. Menezes GC, Elias CN, Attias M. Osteoblast adhesion onto titanium dental implants. Acta Microscopica 2003; 12: 13–20.
18. Chambrone L, Shibli JA, Mercúrio CE, Cardoso B, Preshaw PM. Efficacy of standard (SLA) and modified sandblasted and acid-etched (SLActive) dental implants in promoting immediate and/or early occlusal loading protocols: a systematic review of prospective studies. Clin Oral Implants Res. 2015;26(4):359-70. doi: 10.1111/clr.12347.
19. Zhao G, Schwartz Z, Wieland M, Rupp F, Geis-Gerstorfer J, Cochran DL, Boyan BD. High surface energy enhances cell response to titanium substrate microstructure. J Biomed Mater Res A. 2005;74(1):49-58. doi: 10.1002/jbm.a.30320.
20. Buser D, Nydegger T, Hirt HP, Cochran DL, Nolte LP. Removal torque values of titanium implants in the maxilla of miniature pigs. Int J Oral Maxillofac Implants. 1998;13(5):611-9.
21. Khandelwal N, Oates TW, Vargas A, Alexander PP, Schoolfield JD, Alex McMahan C. Conventional SLA and chemically modified SLA implants in patients with poorly controlled type 2 diabetes mellitus—a randomized controlled trial. Clin Oral Implants Res. 2013;24(1):13-9. doi: 10.1111/j.1600-0501.2011.02369.x.
22. Mastrangelo F, Quaresima R, Canullo L, Scarano A, Muzio LL, Piattelli A. Effects of Novel Laser Dental Implant Microtopography on Human Osteoblast Proliferation and Bone Deposition. Int J Oral Maxillofac Implants. 2020;35(2):320-9. doi: 10.11607/jomi.7606.